

FIG. 1A

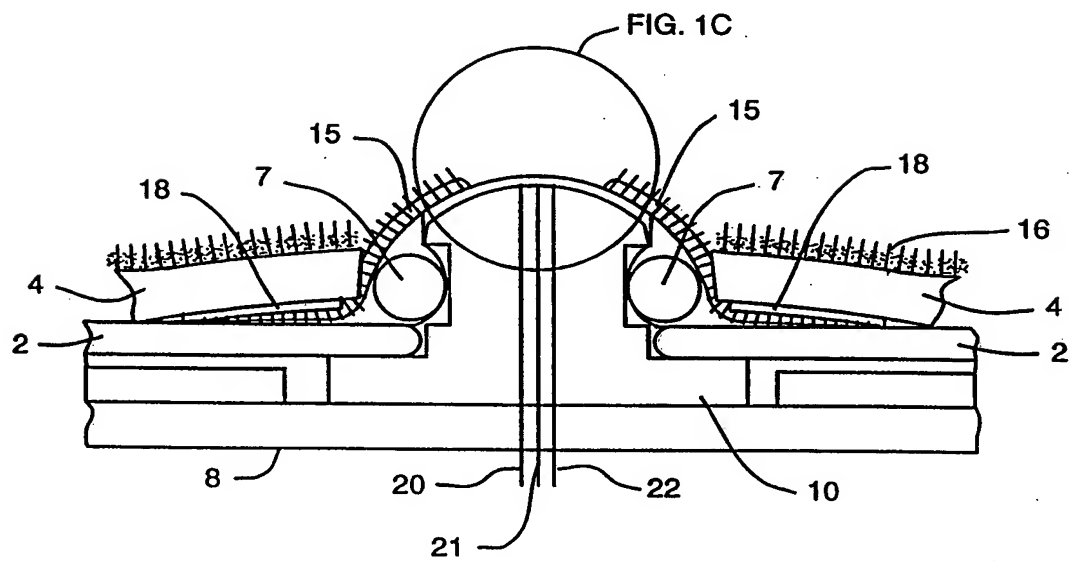


FIG. 1B

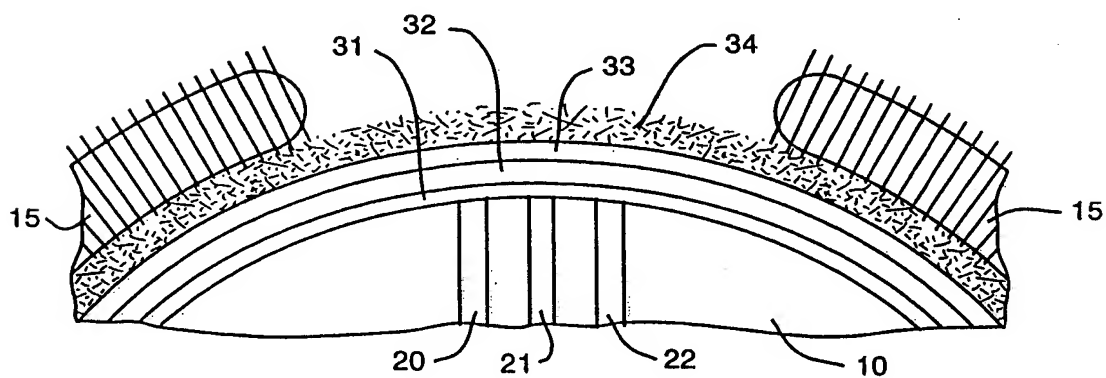


FIG. 1C

DEVICE AND METHOD FOR DETERMINING ANALYTE LEVELS

Shults, et al.

Appl. No.: Unknown

Atty Docket: DEXCOM.8DVC1C1

3/10

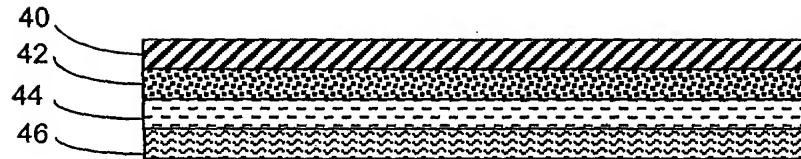


FIG. 1D

4/10

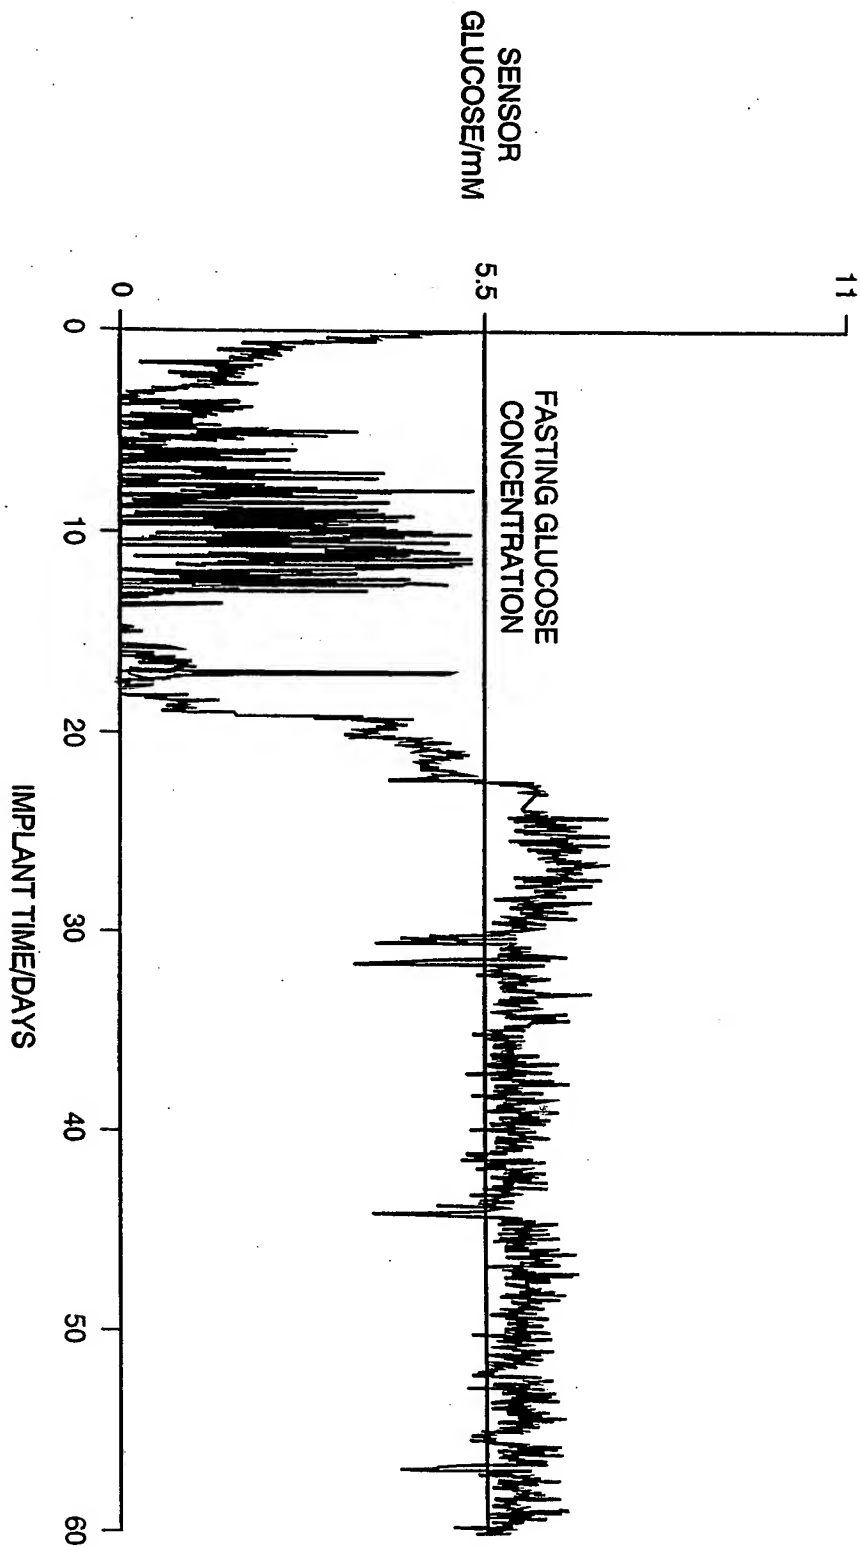


FIG. 2

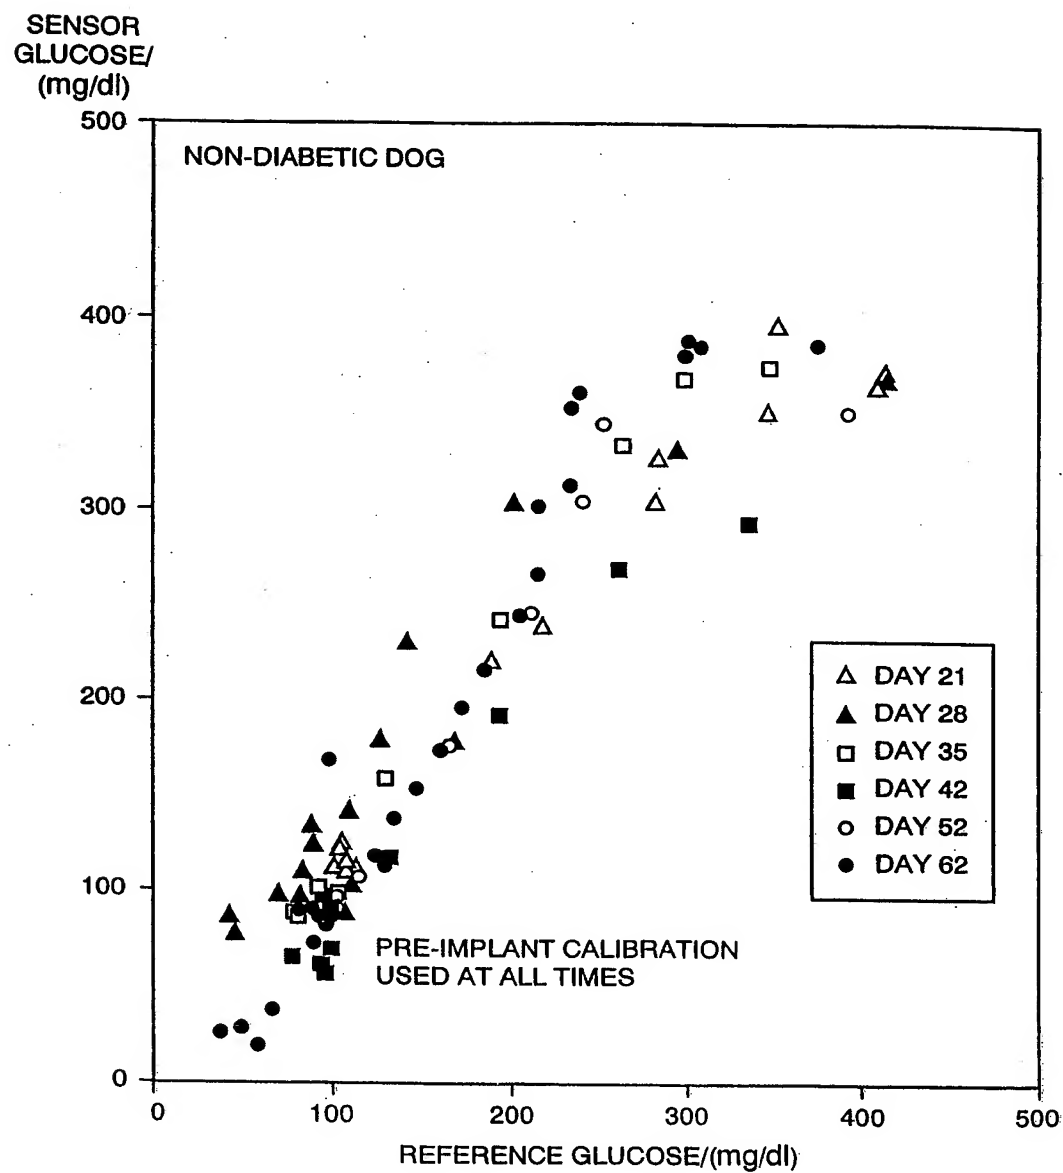


FIG. 3

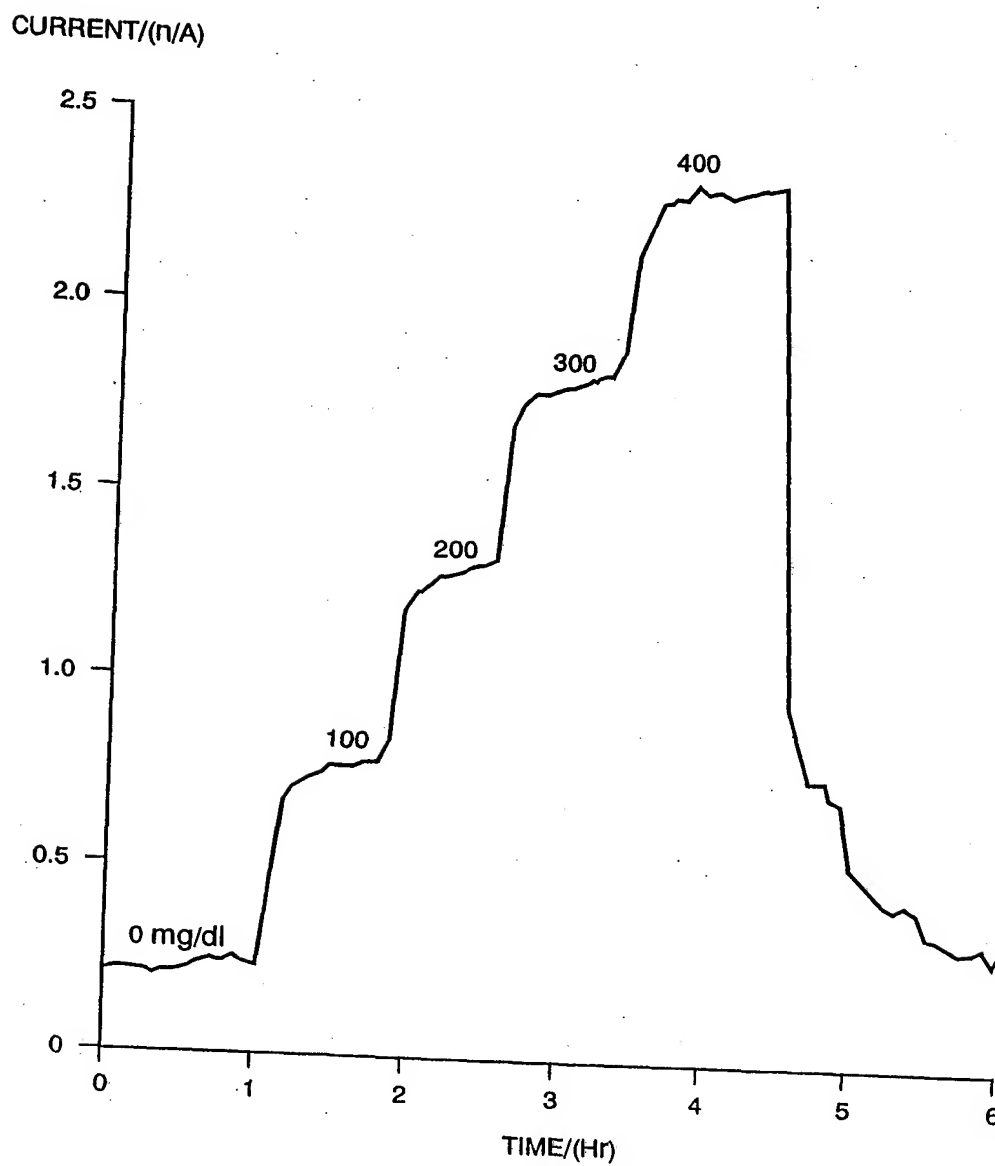


FIG. 4

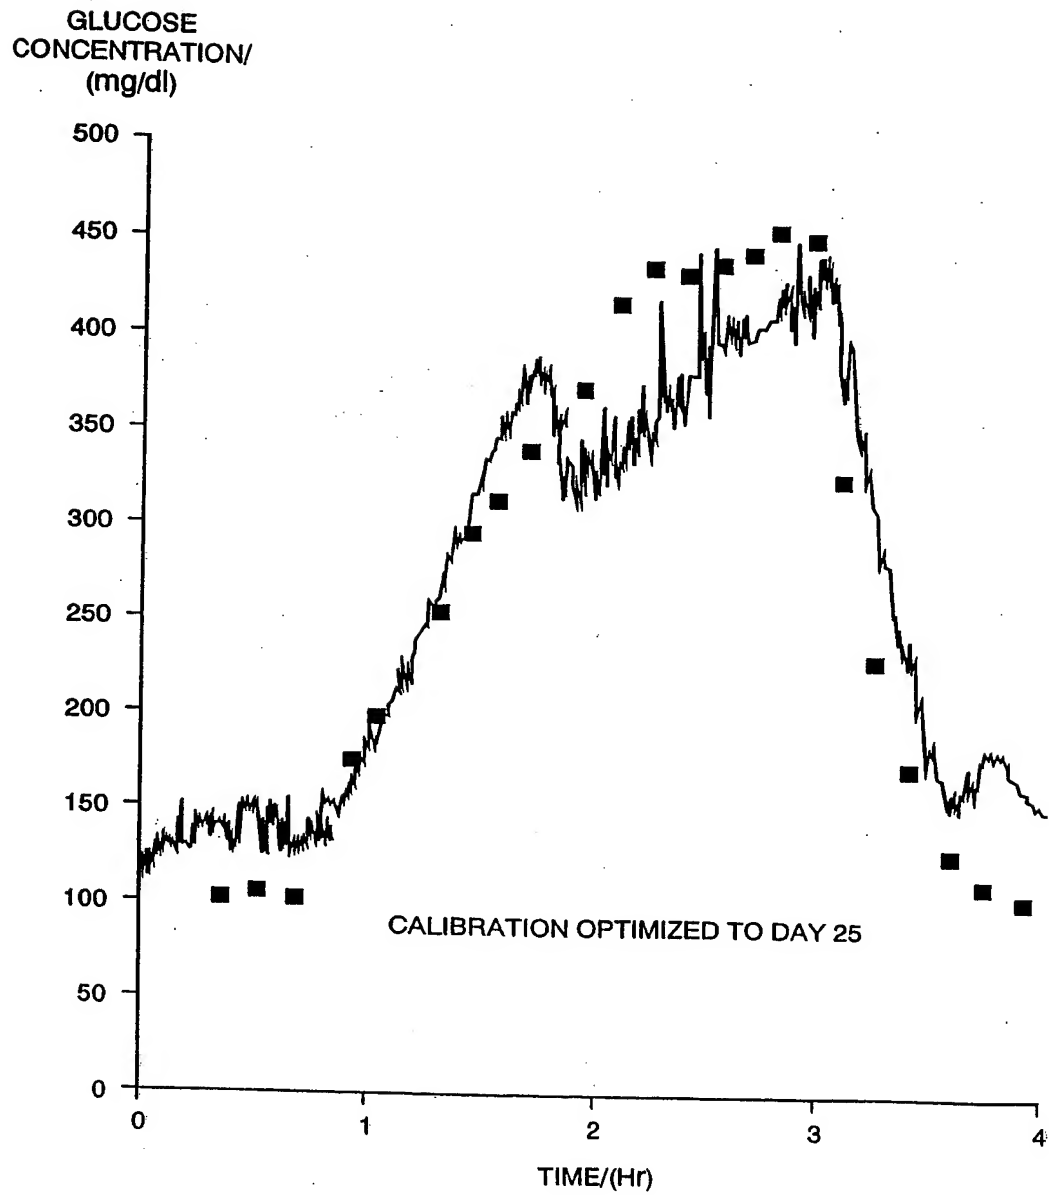


FIG. 5A

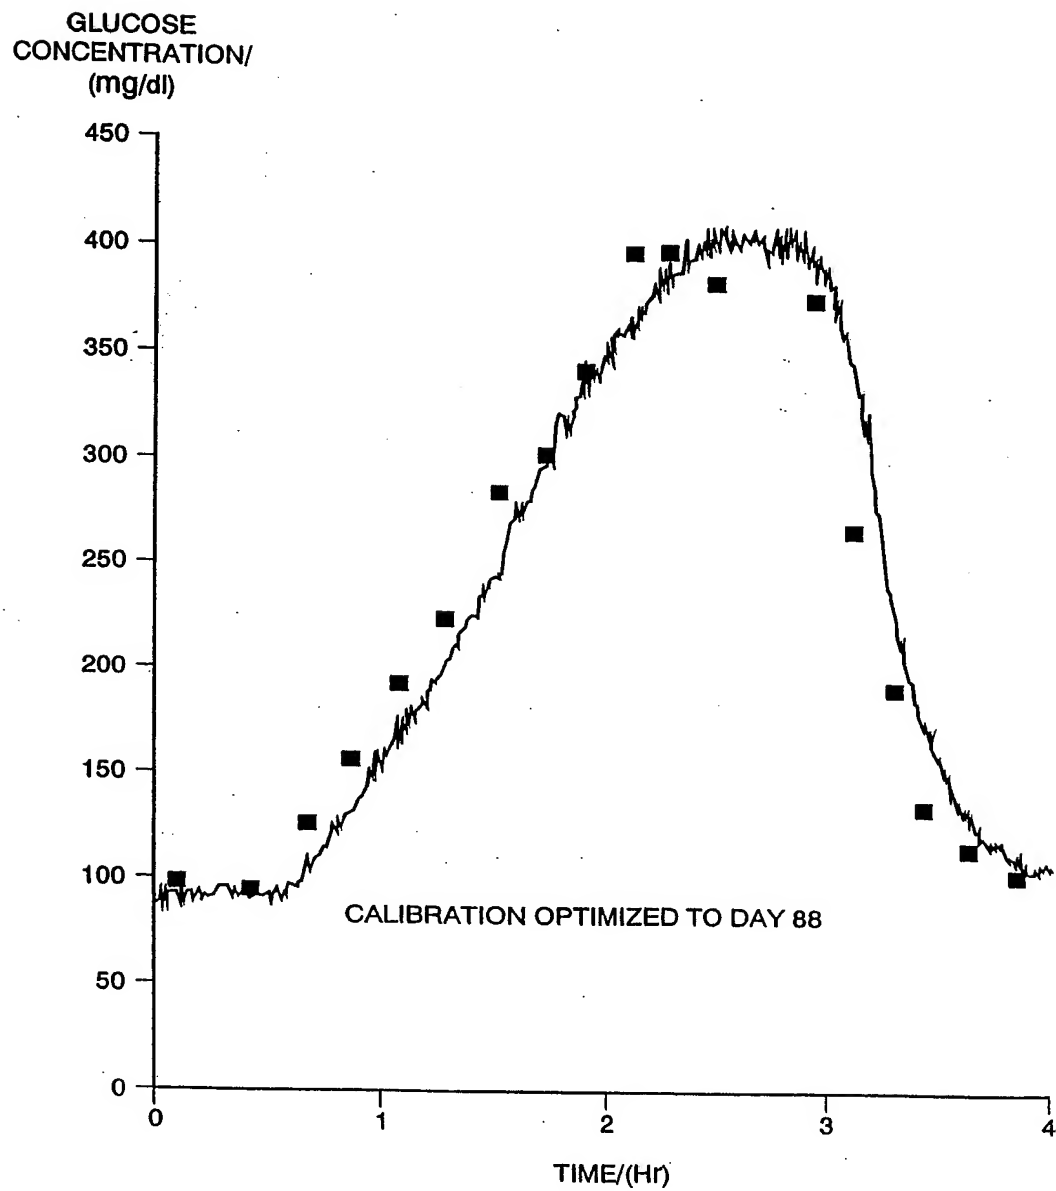


FIG. 5B



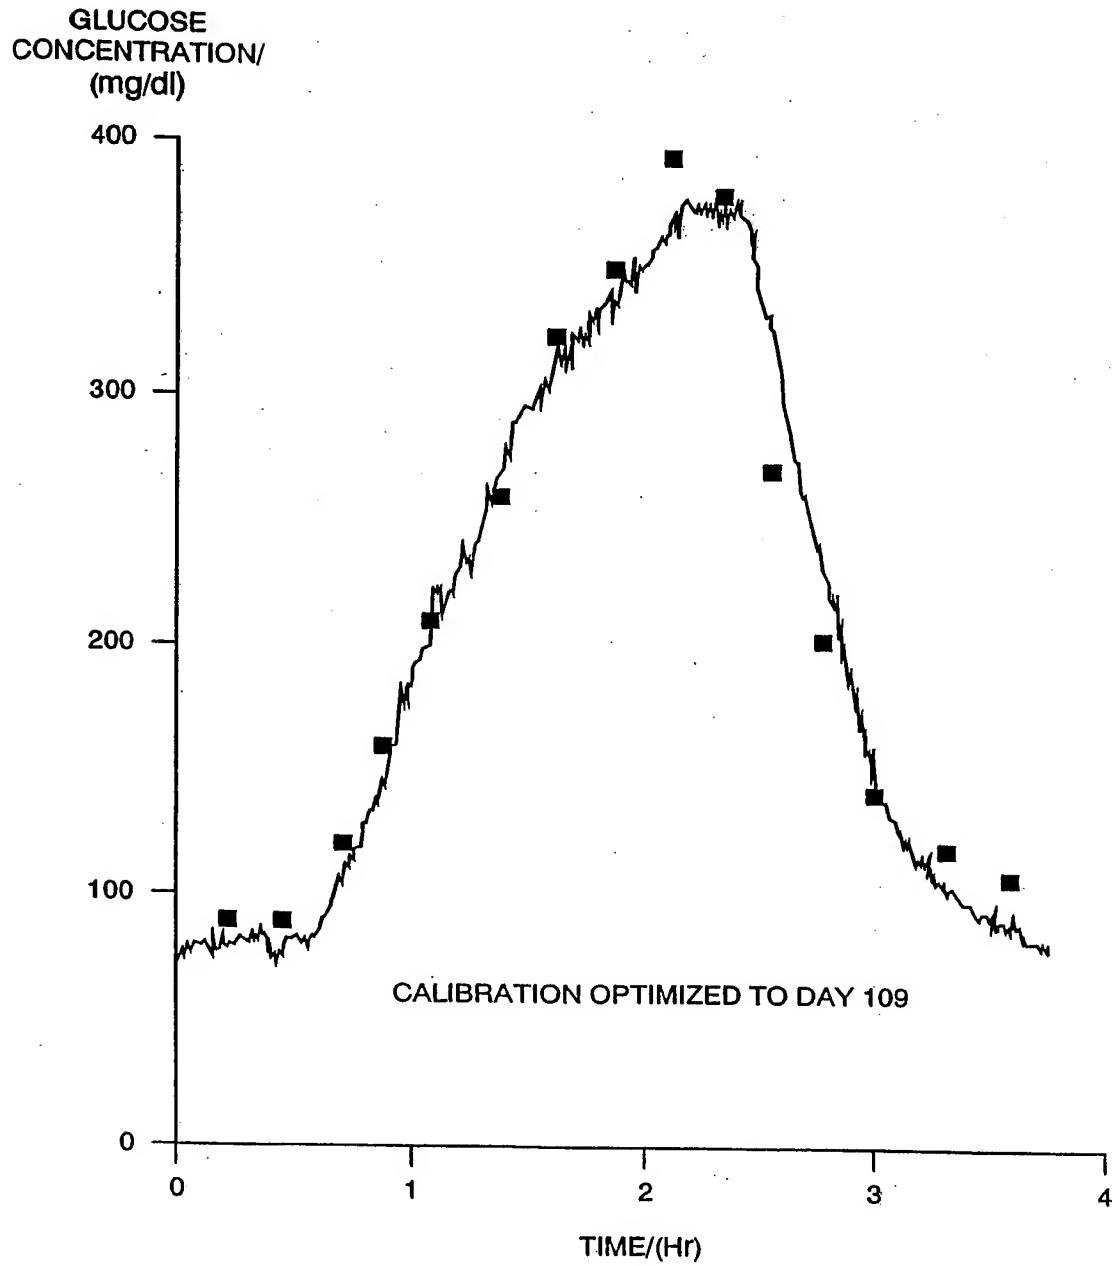


FIG. 5C

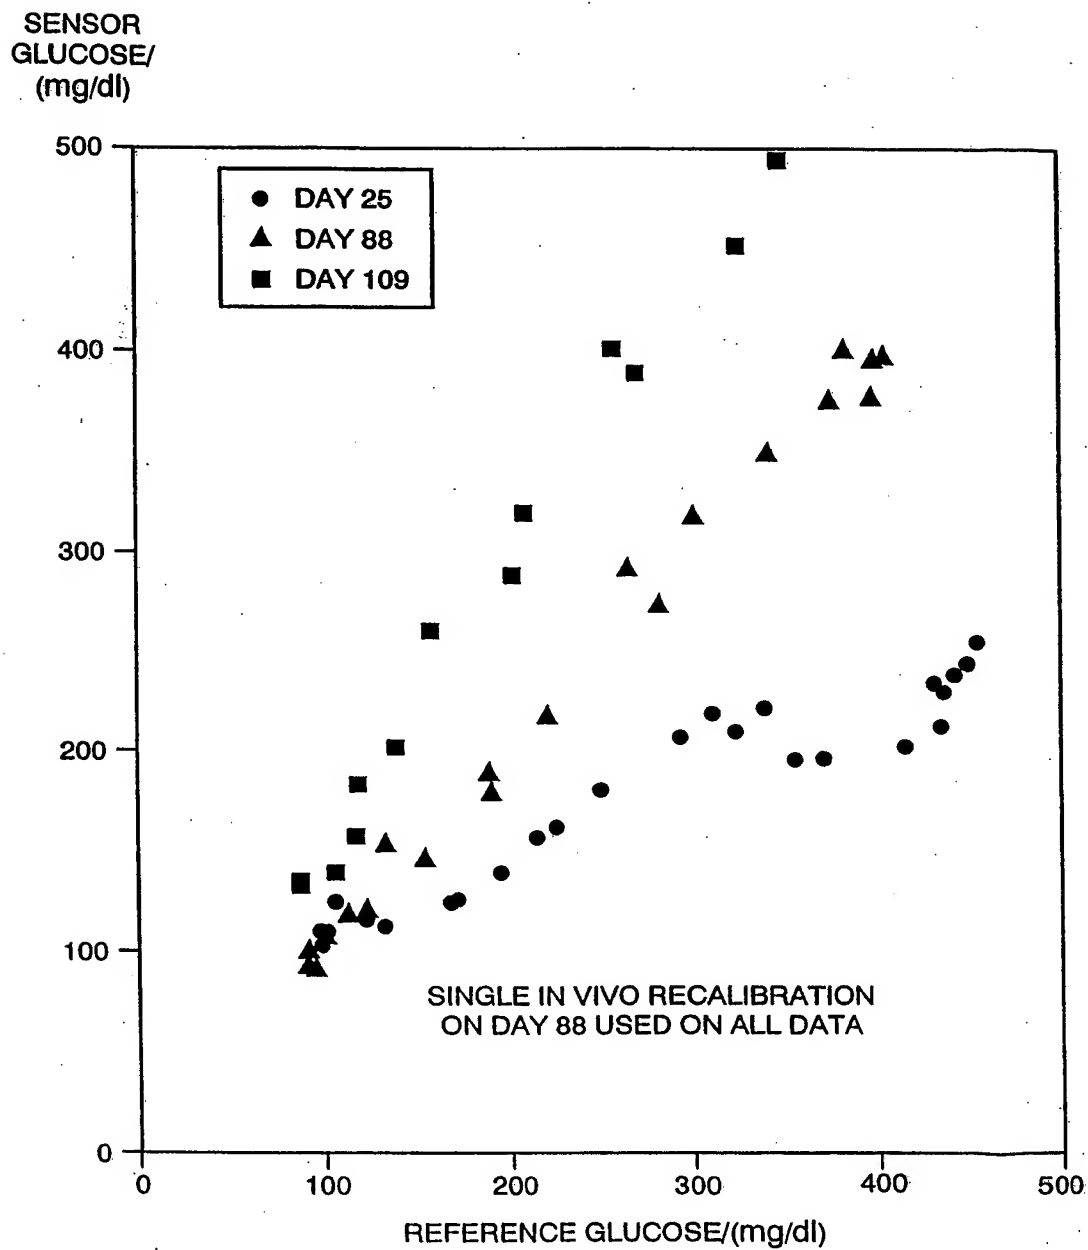


FIG. 6